

## HUMAN STANNIOCALCIN-1 (STC1) ELISA KIT

FOR THE QUANTITATIVE DETERMINATION  
OF HUMAN STC1 CONCENTRATIONS IN  
SERUM AND PLASMA



ALWAYS REFER TO LOT SPECIFIC PROTOCOL  
PROVIDED WITH EACH KIT FOR  
INSTRUCTIONS. PROTOCOL MUST BE  
READ BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN  
DIAGNOSTIC PROCEDURES.

### PURCHASE INFORMATION:

ELISA NAME	HUMAN STC1 ELISA
Catalog No.	SK00157-01
Lot No.	
Formulation	96 T
Standard Range	31.25 - 2000 pg/ml
Sensitivity	10 pg/ml
Sample Volume	100 µl
Sample Type	Serum, EDTA Plasma
Dilution Factor	<b>Optimal dilutions should be determined by each laboratory for each application</b>
Specificity	Human
Calibration	Human STC1 recombinant
Intra-assay Precision	4 - 6%
Inter-assay Precision	8 - 10%
Storage	2 – 8° C
This kit contains sufficient materials to run 35 samples duplicated provided that assay is run according to protocol.	

### Order Contact:

AVISCIERA BIOSCIENCE, INC  
2348 WALSH AVE., SUITE C  
SANTA CLARA, CA 95051  
USA

Tel: 408-982-0300

Fax: 408-982-0301

Email: [Sales@AvisceraBioscience.com](mailto:Sales@AvisceraBioscience.com)

[www.AvisceraBioscience.com](http://www.AvisceraBioscience.com)

**DESCRIPTION**

This Human Stanniocalcin-1 (STC1) ELISA Kit contains the necessary components required for the quantitative measurement of recombinant and/or natural human STC1 from serum and plasma in a sandwich ELISA format.

This immunoassay contains recombinant human STC1 and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural STC1 samples.

**ASSAY OVERVIEW**

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with an antibody specific for human STC1. The capture antibody can bind to the human STC1 in the standard and samples. After washing the plate of any unbound substances, a biotinylated antibody against human STC1 is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution is added to the wells and color develops in direct proportion to the amount of human STC1 bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

**PROCEDURAL LIMITATIONS**

\_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

\_This ELISA kit should not be used beyond the expiration date on the kit label.

\_Do not mix reagents with those from other lots or sources.

\_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

\_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest. If samples generate values that are not within the dynamic range of the standard curve, further concentrate or dilute the samples as required with Dilution Buffer and repeat the assay.

\_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

\_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

**COMPONENTS PROVIDED**

DESCRIPTION	CODE	QUANTITY
<b>STC1 Microplate</b> - 96 well polystyrene microplate (12 strips of 8 wells) coated with an antibody against STC1.	<b>157-01-01</b>	<b>1 plate</b>
<b>STC1 Standard</b> – 2000 pg/vial of recombinant human STC1 in a buffered protein base with preservative; lyophilized.	<b>157-01-02</b>	<b>1 vial</b>
<b>Detection Antibody Concentrate</b> – 1.05 mL/vial, 10-fold concentrate of biotinylated antibody against STC1 with preservative; lyophilized.	<b>157-01-03</b>	<b>1 vial</b>
<b>Positive Control</b> – one vial of recombinant human STC1; lyophilized.	<b>157-01-04</b>	<b>1 vial</b>
<b>Streptavidin-HRP Conjugate</b> - 120 µL/vial, 100-fold concentrated solution of Streptavidin conjugate to HRP.	<b>SAHRP</b>	<b>1 vial</b>
<b>Dilution Buffer</b> – 60 mL of buffered protein based solution with preservative.	<b>DB01</b>	<b>1 bottle</b>
<b>Antibody &amp; HRP Diluent Solution</b> – 30 mL of buffered protein based solution with preservative.	<b>DB08</b>	<b>1 bottle</b>
<b>Wash Buffer</b> - 50 mL of 10-fold concentrated buffered surfactant, with preservative.	<b>WB01</b>	<b>1 bottle</b>
<b>TMB Substrate Solution</b> - 11 mL of TMB substrate solution.	<b>TMB01</b>	<b>1 bottle</b>
<b>Stop Solution</b> – 11 mL of 0.5M HCl.	<b>S-STOP</b>	<b>1 bottle</b>
<b>Plate Sealer</b>	<b>EAPS</b>	<b>1</b>
<b>Plastic Pouch</b>	<b>P01</b>	<b>1</b>

**STORAGE**

**Unopened Kit:** Store at 2 – 8° C for up to 8 months. For longer storage, unopened Standard, Positive Control and Detection Antibody Concentrate should be stored at -20° C or -70° C. Do not use kit past expiration date.

**Opened / Reconstituted Reagents:** Reconstituted Standard (stock) solution and Detection Antibody concentrated Solution SHOULD BE STORED at -20° C

or -70° C for up to one month. Streptavidin-HRP Conjugate 100-fold concentrated solution (protect from light) and other components may be stored at 2 – 8° C for up to 8 months.

**Microplate Wells:** Return unused wells to the plastic pouch with the desiccant pack. Microplate may be stored for up to 6 months at 2 – 8° C after opening.

**ADDITIONAL MATERIALS REQUIRED**

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (250 – 300 rpm).
- Microplate washer or manifold dispenser.
- 100 ml and 500 ml graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

**PRECAUTIONS FOR USE**

All reagents should be considered as potentially hazardous. The stop solution contains diluted hydrochloric acid. Appropriate care, therefore, should be taken while handling this solution. We therefore recommend that this product is handled only by those persons who have been trained in laboratory techniques and that it is used in accordance with the principles of good laboratory practice. Wear suitable protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken to avoid contact with skin or eyes. In the case of contact with skin or eyes wash immediately with water.

**SAMPLE COLLECTION AND STORAGE**

**Serum** - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

**Plasma** - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

**Optional: Use Aprotinin (enzyme inhibitor) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.**

**SAMPLE PREPARATION**

Serum and plasma samples DO NOT need to be diluted. **Optimal dilutions should be determined by each laboratory for each application.**  
**Use polypropylene test tubes.**


**REAGENT PREPARATION**

**Bring all reagents to room temperature before use.**

**Wash Buffer** - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into deionized or distilled water (450 mL) to prepare 500 mL of 1x Wash Buffer.

**STC1 Standard** - Reconstitute the STC1 standard with 1.0 mL of Dilution Buffer. This reconstitution produces a stock solution of 2000 pg/ml. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 250 µl of Dilution Buffer into tubes #1 to #6. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The **2000 pg/ml** standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 pg/ml).

Tube	Standard	Dilution Buffer	Concentration
Stock	Powder	1.0 ml	2000 pg/ml
# 1	250 µl of stock	250 µl	1000 pg/ml
# 2	250 µl of 1	250 µl	500 pg/ml
# 3	250 µl of 2	250 µl	250 pg/ml
# 4	250 µl of 3	250 µl	125 pg/ml
# 5	250 µl of 4	250 µl	62.5 pg/ml
# 6	250 µl of 5	250 µl	31.2 pg/ml

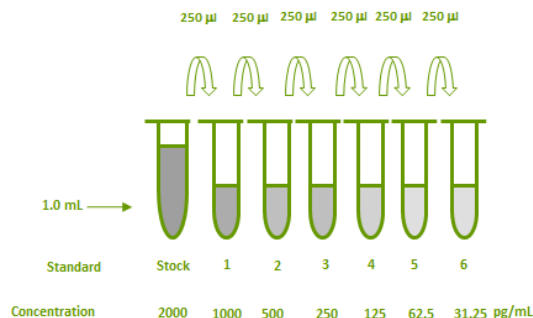

**Positive Control** - Reconstitute the Positive Control with 1.0 mL of Dilution Buffer. **Note:** *Positive Control could be reused within a few days if stored at -20° C or -70° C.*

**Detection Antibody** - Reconstitute the Detection Antibody Concentrate with 1.05 mL of **Antibody & HRP Diluent Solution (DB08)** to produce a 10-fold concentrated stock solution. Pipette 9.45 mL of Antibody & HRP Diluent Solution (DB08) into a 15 mL centrifuge tube and transfer 1.05 mL of 10-fold concentrated stock solution to prepare working solution.

**Streptavidin-HRP Conjugate** - Pipette 11.88 mL of **Antibody & HRP Diluent Solution (DB08)** into a 15 mL centrifuge tube and transfer 120 µl of 100-fold concentrated stock solution to prepare working solution. **(Protect from light.) Note:** *1x working solution of Streptavidin-HRP Conjugate should be used within a few days.*

## ELISA PROTOCOL

**Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.**

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the plastic pouch with the desiccant pack.
3. Add 100 µl of **Dilution Buffer** to Blank wells.
4. Add 100 µl of **Standard dilutions (#6-#S, reverse order of serial dilution), samples, or positive control** per well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
5. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with **1x Wash Buffer** (300 µl) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 100 µl of **Detection Antibody working solution** to each well. Cover with plate sealer.

Incubate for 2 hours on microplate shaker at room temperature.

7. Repeat the aspiration/wash as in step 5.
8. Add 100 µl of **Streptavidin-HRP Conjugate working solution** to each well. Incubate for 45 minutes on microplate shaker at room temperature. **Protect from light.**
9. Repeat the aspiration/wash as in step 5.
10. Add 100 µl of **Substrate Solution** to each well. Incubate for 3-7 minutes on microplate shaker at room temperature. **Protect from light.**
11. Add 100 µl of **Stop Solution** to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Determine the optical density of each well within 15 minutes, using a microplate reader set to 450 nm.

## CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log curve fit to more accurately quantify the standard dilutions.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

Calculation of samples with a concentration exceeding that of standard 2000 pg/mL may result in inaccurate, low human STC1 levels. Such samples require further external predilution according to expected human STC1 values with Dilution Buffer in order to precisely quantify the actual human STC1 level.

## SPECIFICITY

PROTEINS	CROSS-REACTIVITY (%)
Human STC1	100
Human Biglycan	0
Human Decorin	0

**TYPICAL DATA**

This standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

STC1 (pg/ml)	Average OD450 (Corrected)*
Blank	0 (0.066)
31.25	0.031
62.5	0.046
125	0.100
250	0.227
500	0.401
1000	0.658
2000	0.962

- Lot No.:
- Positive Control:

**SUMMARY OF ASSAY PROCEDURE**

PREPARE REAGENTS, SAMPLES AND STANDARDS
↓
Add 100 µl of standard dilutions, samples, or positive control to the well. Incubate 2 hours on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Detection Antibody working solution to each well. Incubate 2 hours on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Streptavidin-HRP conjugate working solution to each well. Incubate 45 minutes on the plate shaker at RT. <b>Protect from light.</b>
↓
Aspirate and wash 4 times.
↓
Add 100 µl Substrate Solution to each well. Incubate 3-7 minutes on the plate shaker at RT. <b>Protect from light.</b>
↓
Add 100 µl Stop Solution to each well. Read 450nm within 15 min.