

HUMAN CORIN ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF HUMAN CORIN CONCENTRATIONS IN CELL CULTURE SUPERNATES, SERUM, AND PLASMA.



FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

PURCHASE INFORMATION:

ELISA Name	Human CORIN ELISA
Catalog No.	SK00695-01
Formulation	96 T
Standard range	62.5-4000 pg/ml
Sensitivity	15-31 pg/ml
Sample Volume	100 μ l
Sample Type	Serum, EDTA Plasma, cell culture
Dilution Factors	<i>Optimal dilutions should be determined by each laboratory for each application.)</i>
Specificity	Human CORIN only
Intra-assay Precision	4-6%
Inter-assay Precision	8-10%
Storage	2 °C-8 °C

Order Contact:

AVISCERA BIOSCIENCE INC.

2348 Walsh Ave., Suite C

Santa Clara, CA 95051

Tel: (408) 982 0300

Fax: (408) 982 0301

Email: Sales@AvisceraBioscience.com

Info@AvisceraBioscience.com

www.AvisceraBioscience.com

INTRODUCTION

Human CORIN immunoassay is a 3.5 - 4.5 hour solid phase ELISA designed to measure human CORIN in cell culture supernates, serum, and plasma. It contains recombinant human CORIN and antibodies raised against this protein. It has been shown to accurately quantitate recombinant human CORIN. Results obtained with naturally occurring CORIN samples showed linear curves that were parallel to the standard curves obtained using the kit standards. These results indicate that the Immunoassay kit can be used to determine relative mass values for natural human CORIN.

PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. A monoclonal antibody specific for CORIN has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any CORIN present is bound by the immobilized antibody. After washing away any unbound substances, a biotinylated polyclonal antibody specific for CORIN is added to the wells. Following a wash to remove any unbound antibody-biotin reagent, HRP link Streptavidin is added to the wells. After washing away any unbound enzyme, a substrate solution is added to the wells and color develops in proportion to the amount of CORIN bound in the initial step. The color development is stopped and the intensity of the color is measured.

LIMITATIONS OF THE PROCEDURE

_ FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_ The kit should not be used beyond the expiration date on the kit label.

_ Do not mix or substitute reagents with those from other lots or sources.

_ It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_ If samples generate values higher than the highest standard, dilute the samples with the appropriate Dilution Buffer and repeat the assay.

_ Any variation in standard diluent, operator, pipetting technique, washing technique, incubation time or temperature, and kit age can cause variation in binding.

_ This assay is designed to eliminate interference by soluble receptors, binding proteins, and other factors present in biological samples. Until all factors

have been tested in the Immunoassay, the possibility of interference cannot be excluded.

MATERIALS PROVIDED

Description	Code	Quantity
CORIN Microplate - 96 well polystyrene microplate (12 strips of 8 wells) coated with a purified monoclonal antibody against human CORIN.	695-01-01	1 plate
CORIN Standard – 4000pg/vial of recombinant human CORIN in a buffered protein base with preservatives; lyophilized.	695-01-02	1 vial
Detection Antibody Concentrate – 120 µL / vial, 100-fold concentrated of Biotinylated polyclonal antibody against CORIN with preservatives; lyophilized.	695-01-03	1 vial
Positive Control - one of recombinant human CORIN, lyophilized	695-01-04	1 vial
Streptavidin-HRP Conjugate -120 ul/vial, 100-fold concentrated solution of Streptavidin conjugate to HRP	SAHRP	1 vial
Dilution Buffer - 60mL/vial of buffered protein based solution with preservatives	DB01	1 vial
Wash Buffer -50 ml/vial, 10-fold concentrated buffered surfactant, with preservative.	WB01	1 vial
TMB Substrate Solution -13 ml / vial of TMB substrate solution	TMB01	1 vial
Stop Solution (0.5M HCl) , 13 ml /vial of 0.5M HCl	S-STOP	1 vial
Plate Covers – Plate sealer.	EAPS	1

STORAGE

Unopened Kit: Store at 2 - 8° C for up to 6 months. For longer storage, unopened Standard, Positive

Control and Detection Antibody Concentrated should be stored at -20 or -70 °C. Do not use past kit expiration date.

Opened / Reconstituted Reagents: *Reconstituted Standard (4ng/ml), Antibody Solution SHOULD BE STORED at -20 °C or -70°C for up to one months.* Streptavidin - HRP Conjugate 100-fold concentrated and other components may be stored at 2 - 8°C for up to 6 months. *Reconstituted Positive Control should be prepared and used immediately.*

Microplate Wells: Return unused wells to the plastic bag containing the desiccant pack, reseal along entire edge of zip-seal. May be stored for up to 6 months at 2 - 8° C.

OTHER SUPPLIES REQUIRED

- Microplate reader capable of measuring absorbance at 450 nm, with the correction wavelength set at 540 nm or 570 nm.
- Microplate shaker (250-300rpm).
- Pipettes and pipette tips.
- Deionized or distilled water.
- Squirt bottle, manifold dispenser, or automated microplate washer.
- 100 mL and 500 mL graduated cylinders.

PRECAUTIONS FOR USE

All reagents should be considered as potentially hazardous. The stop solution contains diluted Hydrochloric acid. Appropriate care, therefore, should be taken while handling this solution. We therefore recommend that this product is handled only by those persons who have been trained in laboratory techniques and that it is used in accordance with the principles of good laboratory practice. Wear suitable protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken to avoid contact with skin or eyes. In the case of contact with skin or eyes wash immediately with water.

SAMPLE COLLECTION AND STORAGE

Cell Culture Supernates - Remove particulates by centrifugation and assay immediately or aliquot and store samples at ≤-20° C. Avoid repeated freeze-thaw cycles.

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay

immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Plasma - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤-20° C. Avoid repeated freeze-thaw cycles.

SAMPLE PREPARATION

Optimal dilutions should be determined by each laboratory for each application.

Use polypropylene test tubes.


REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into deionized or distilled water (450 mL) to prepare 500 mL of Wash Buffer.

CORIN Standard - Refer to vial label for reconstitution volume. Reconstitute the **CORIN** Standard with 1 ml of Dilution Buffer. This reconstitution produces a stock solution of 4000 pg/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 250 µL of the appropriate Dilution Buffer into the tube #1 to #6. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The 4000 pg/mL standard serves as the high standard. The appropriate Dilution Buffer serves as the zero standard (0 pg/mL).

Standard	Standard	Reagent Diluent	Concentration
stock	Powder	1000 µl	4000 pg/ml
# 1	250 µl of stock	250 µl	2000 pg/ml
# 2	250 µl of 1	250 µl	1000 pg/ml
# 3	250 µl of 2	250 µl	500 pg/ml
# 4	250 µl of 3	250 µl	250 pg/ml
# 5	250 µl of 4	250 µl	125 pg/ml
# 6	250 µl of 5	250 µl	62.5 pg/ml

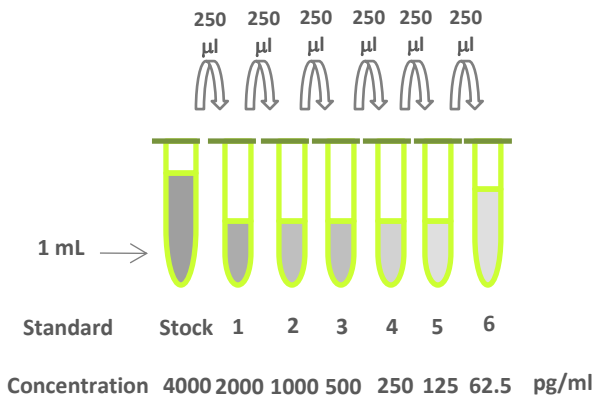

Detection Antibody- Reconstitute the **Detection Antibody concentrated** with 120 μL of Dilution Buffer to produce a 100-fold concentrated stock solution. Pipette 11.88 mL of the appropriate Dilution Buffer into the 15 ml centrifuge tube and transfer 120 μL of 100-fold concentrated stock solution to prepare working solution.

Streptavidin-HRP Conjugate - Pipette 11.88 mL of Dilution Buffer into the 15 ml centrifuge tube and transfer 120 μL of 100-fold concentrated stock solution to prepare working solution. *Note: 1 x working solution of Streptavidin-HRP Conjugate should be used within a few days.*

Positive Control- Reconstitute the **Positive Control** with 1.0 mL of Dilution Buffer. *Positive Control should be prepared and used immediately.*

ASSAY PROCEDURE

Bring all reagents and samples to room temperature before use. It is recommended that standards be assayed in duplicate.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess micro-plate strips from the plate frame, return them to the foil pouch containing the desiccant pack, reseal.
3. Add 100 μL of Dilution Buffer to Blank well (F4, F5).
4. Add 100 μL of Standard (from B2 to G3, G4 to G5), sample, or positive control per well. Cover with the Sealer. Incubate for 2 hours on micro-plate shaker at room temperature. A plate layout is provided to record standards and samples assayed.
5. Aspirate each well and wash, repeating the process three times for a total of four washes.

Wash by filling each well with Wash Buffer (300 μL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

6. Add 100 μL of Detection Antibody working solution to each well. Cover with sealer. Incubate for 2 hours on micro-plate shaker at room temperature.
7. Repeat the aspiration/wash as in step 5.
8. Add 100 μL of **Streptavidin-HRP Conjugate** to each well. Incubate it on microplate shaker for 45 minutes at room temperature.
9. Repeat the aspiration/wash as in step 5.
10. Add 100 μL of Substrate Solution to each well. Incubate for 5-15 minutes at room temperature. **Protect from light.**
11. Add 100 μL of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Determine the optical density of each well within 15 minutes, using a micro-plate reader set to 450 nm.

CALCULATION OF RESULTS

Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density. Create a standard curve by reducing the data using computer software capable of generating a log-log curve fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the CORIN concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

Calculation of samples with a concentration exceeding that of standard 4000 pg/ml may result in inaccurate, low human CORIN levels. Such samples require further external predilution according to expected human CORIN values with Dilution Buffer

in order to precisely quantitate the actual human CORIN level.

TYPICAL DATA

These standard curves* are provided for demonstration only. A standard curve should be generated for each set of samples assayed.

Standard (pg/mL)	Average OD450 (Corrected)
62.5	0.032
125	0.054
250	0.134
500	0.266
1000	0.552
2000	1.058
4000	2.261

CALIBRATION

This immunoassay is calibrated against a highly purified NS0-expressed recombinant human CORIN.

SPECIFICITY

This assay recognizes both natural and recombinant human CORIN. The factors listed below were prepared at 50 ng/mL in Dilution Buffer, and assayed for cross reactivity.

Proteins	Cross-reactivity (%)
CORIN	100
Gas6	0
AXL	0
PTX-3	0
Galectin-3	0
Fetuin A	0
sRAGE	0
Endothelial Lipase	0

SUMMARY OF ASSAY PROCEDURE

